

Client **Eden Scientific**

 Received **02/03/2026**

 Analyzed **02/08/2026**

This Certificate of Analysis certifies that the sample listed herein was tested by Kovera Labs using validated analytical methods and was found to meet the stated specifications at the time of analysis.

SAMPLE INFORMATION

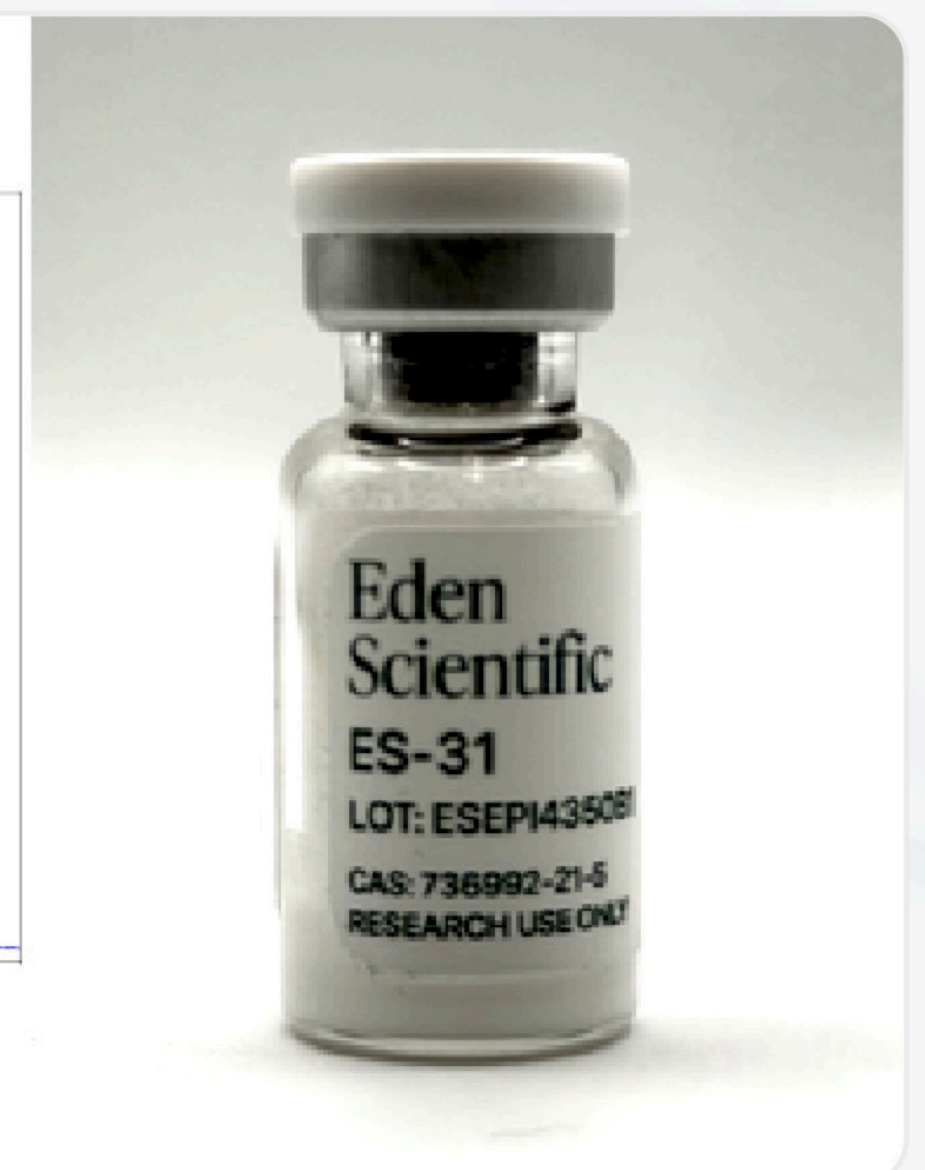
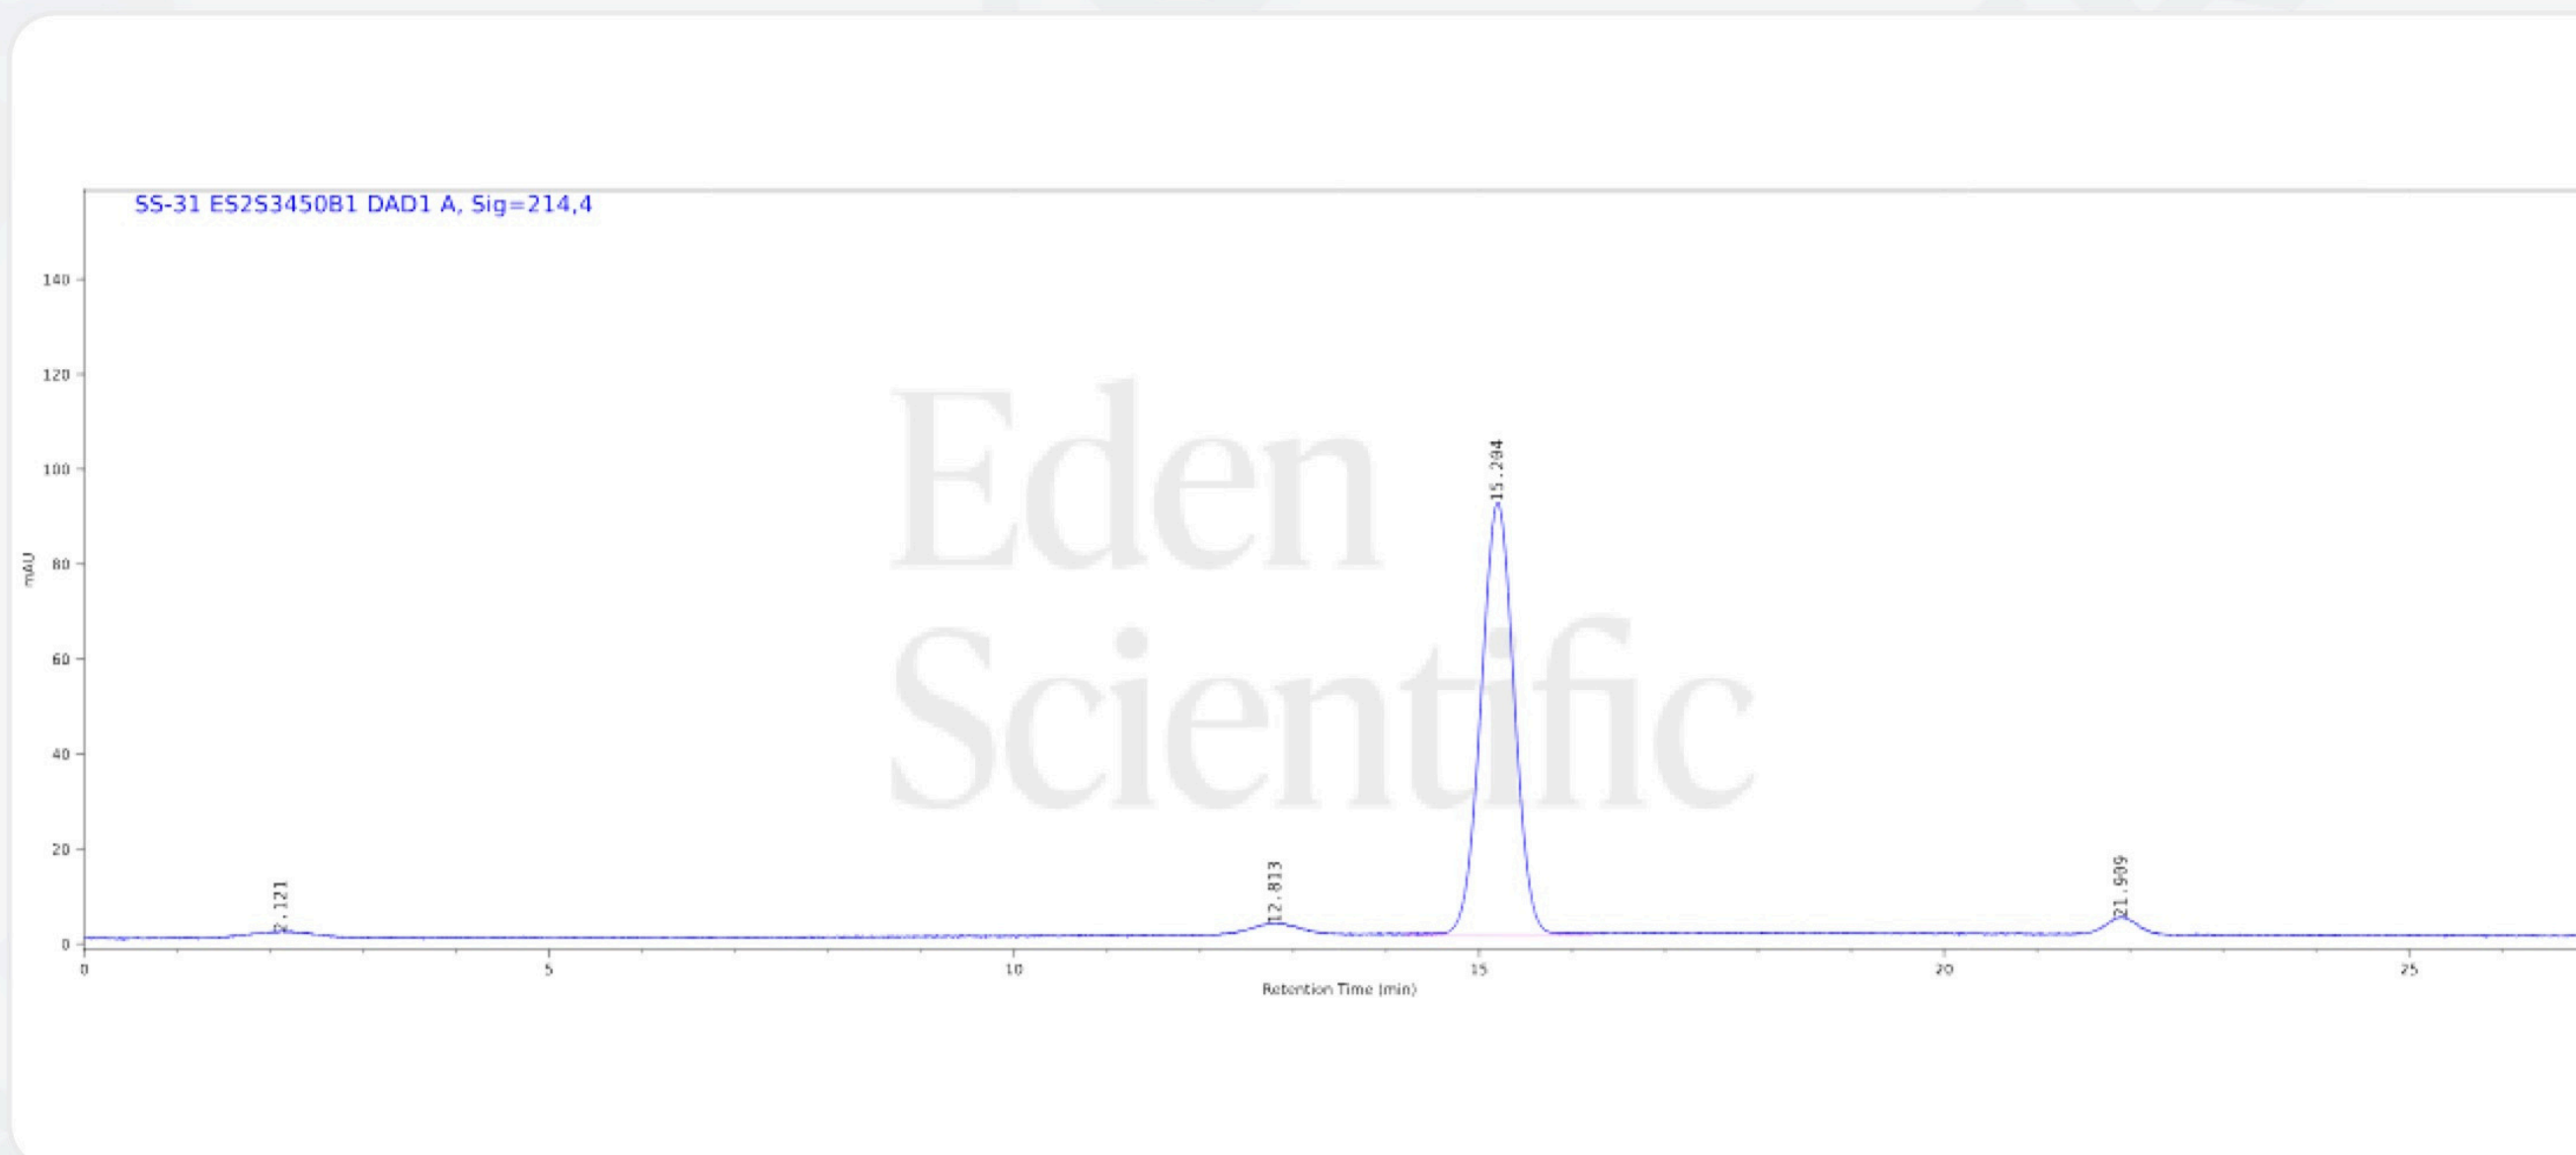
Product	SS-31	Form	Lyophilized powder
Batch	ES2S3450B1	Labeled Qty	35 mg
Mol. Formula	C32H49N5O7	CAS Number	736992-21-5

TEST RESULTS

	REFERENCE STANDARD	RESULT
Purity	(>98%)	99.49% <input checked="" type="checkbox"/>
Net Content	(35mg ± 10%)	37.96 mg <input checked="" type="checkbox"/>
Identity Confirmation (LC-MS)	(SS-31)	SS-31 <input checked="" type="checkbox"/>

CHROMATOGRAM

Method: RP-HPLC / Column: C18 / Detection: DAD @ 214 nm


 David Cohen
 Lab Director

koveralabs.com/verify

Report#: KVR-2026-570445

Access Code: None

CLIENT & SAMPLE INFORMATION

CLIENT	Eden Scientific	PRODUCT NAME	SS-31
CAS NUMBER	736992-21-5	LOT / BATCH	ES2S3450B1
SAMPLE QUANTITY	35 mg	FORM	Lyophilized powder
TEST DATE	02/11/2026		

This Certificate of Analysis certifies that the sample listed herein was tested for microbial sterility screen in accordance with standard laboratory procedures.

TEST RESULTS

TEST	SPECIFICATION	RESULT	STATUS
Microbial Sterility Screen	No growth	No growth detected	PASS

AUTHORIZATION

PREPARED BY

Maya Quinn, B.S.

QC Analyst

REVIEWED BY

David Cohen, M.S.

Quality Director



CLIENT & SAMPLE INFORMATION

CLIENT	Eden Scientific	PRODUCT NAME	SS-31
CAS NUMBER	736992-21-5	LOT / BATCH	ES2S3450B1
SAMPLE QUANTITY	35 mg	FORM	Lyophilized powder
TEST DATE	02/11/2026		

This Certificate of Analysis certifies that the sample listed herein was tested for endotoxin safety screen in accordance with standard laboratory procedures.

TEST RESULTS

TEST	SPECIFICATION	RESULT	STATUS
Endotoxin Safety Screen	≤0.5 EU/mL	PASS	PASS

AUTHORIZATION

PREPARED BY

Marcus Sterling, B.S.

QC Analyst

REVIEWED BY

David Cohen, M.S.

Quality Director



CLIENT & SAMPLE INFORMATION

CLIENT	Eden Scientific	PRODUCT NAME	SS-31
CAS NUMBER	736992-21-5	LOT / BATCH	ES2S3450B1
SAMPLE QUANTITY	35 mg	FORM	Lyophilized powder
TEST DATE	02/11/2026		

This Certificate of Analysis certifies that the sample listed herein was tested for heavy metals screen in accordance with standard laboratory procedures.

HEAVY METALS SCREEN

ELEMENT	SPECIFICATION	RESULT
Lead (Pb)	< LOD	Negative
Cadmium (Cd)	< LOD	Negative
Arsenic (As)	< LOD	Negative
Mercury (Hg)	< LOD	Negative

AUTHORIZATION

PREPARED BY

Liam Clarke, B.S.

QC Analyst

REVIEWED BY

David Cohen, M.S.

Quality Director

