

Client **Eden Scientific**

 Received **02/03/2026**

 Analyzed **02/08/2026**

This Certificate of Analysis certifies that the sample listed herein was tested by Kovera Labs using validated analytical methods and was found to meet the stated specifications at the time of analysis.

SAMPLE INFORMATION



Product	Epithalon	Form	Lyophilized powder
Batch	ESEPI4350B1	Labeled Qty	40 mg
Mol. Formula	C14H22N4O9	CAS Number	307297-39-8

TEST RESULTS

	REFERENCE STANDARD	RESULT
Purity	(>98%)	99.33% <input checked="" type="checkbox"/>
Net Content	(40mg ± 10%)	43.71 mg <input checked="" type="checkbox"/>
Identity Confirmation (LC-MS)	(Epithalon)	Epithalon <input checked="" type="checkbox"/>

CHROMATOGRAM

Method: RP-HPLC | Column: C18 | Detection: DAD @ 214 nm

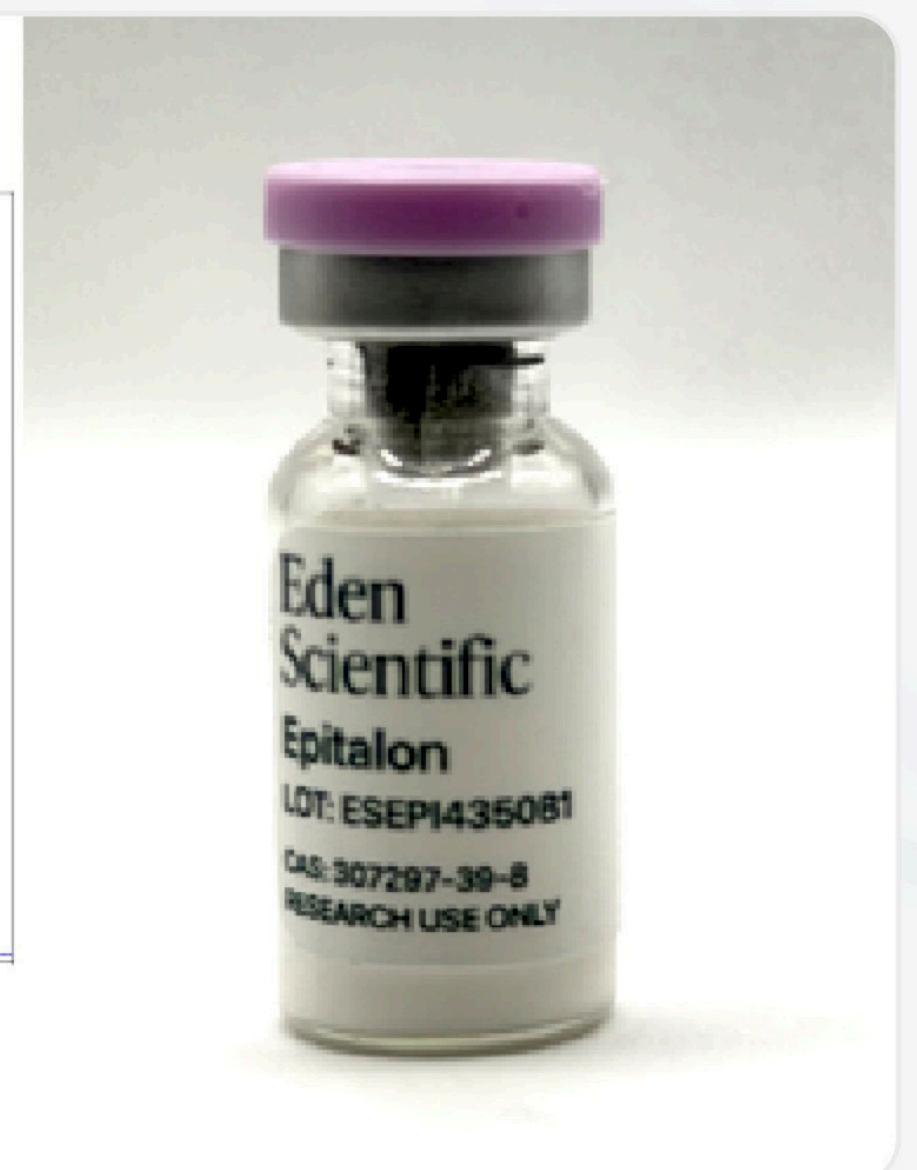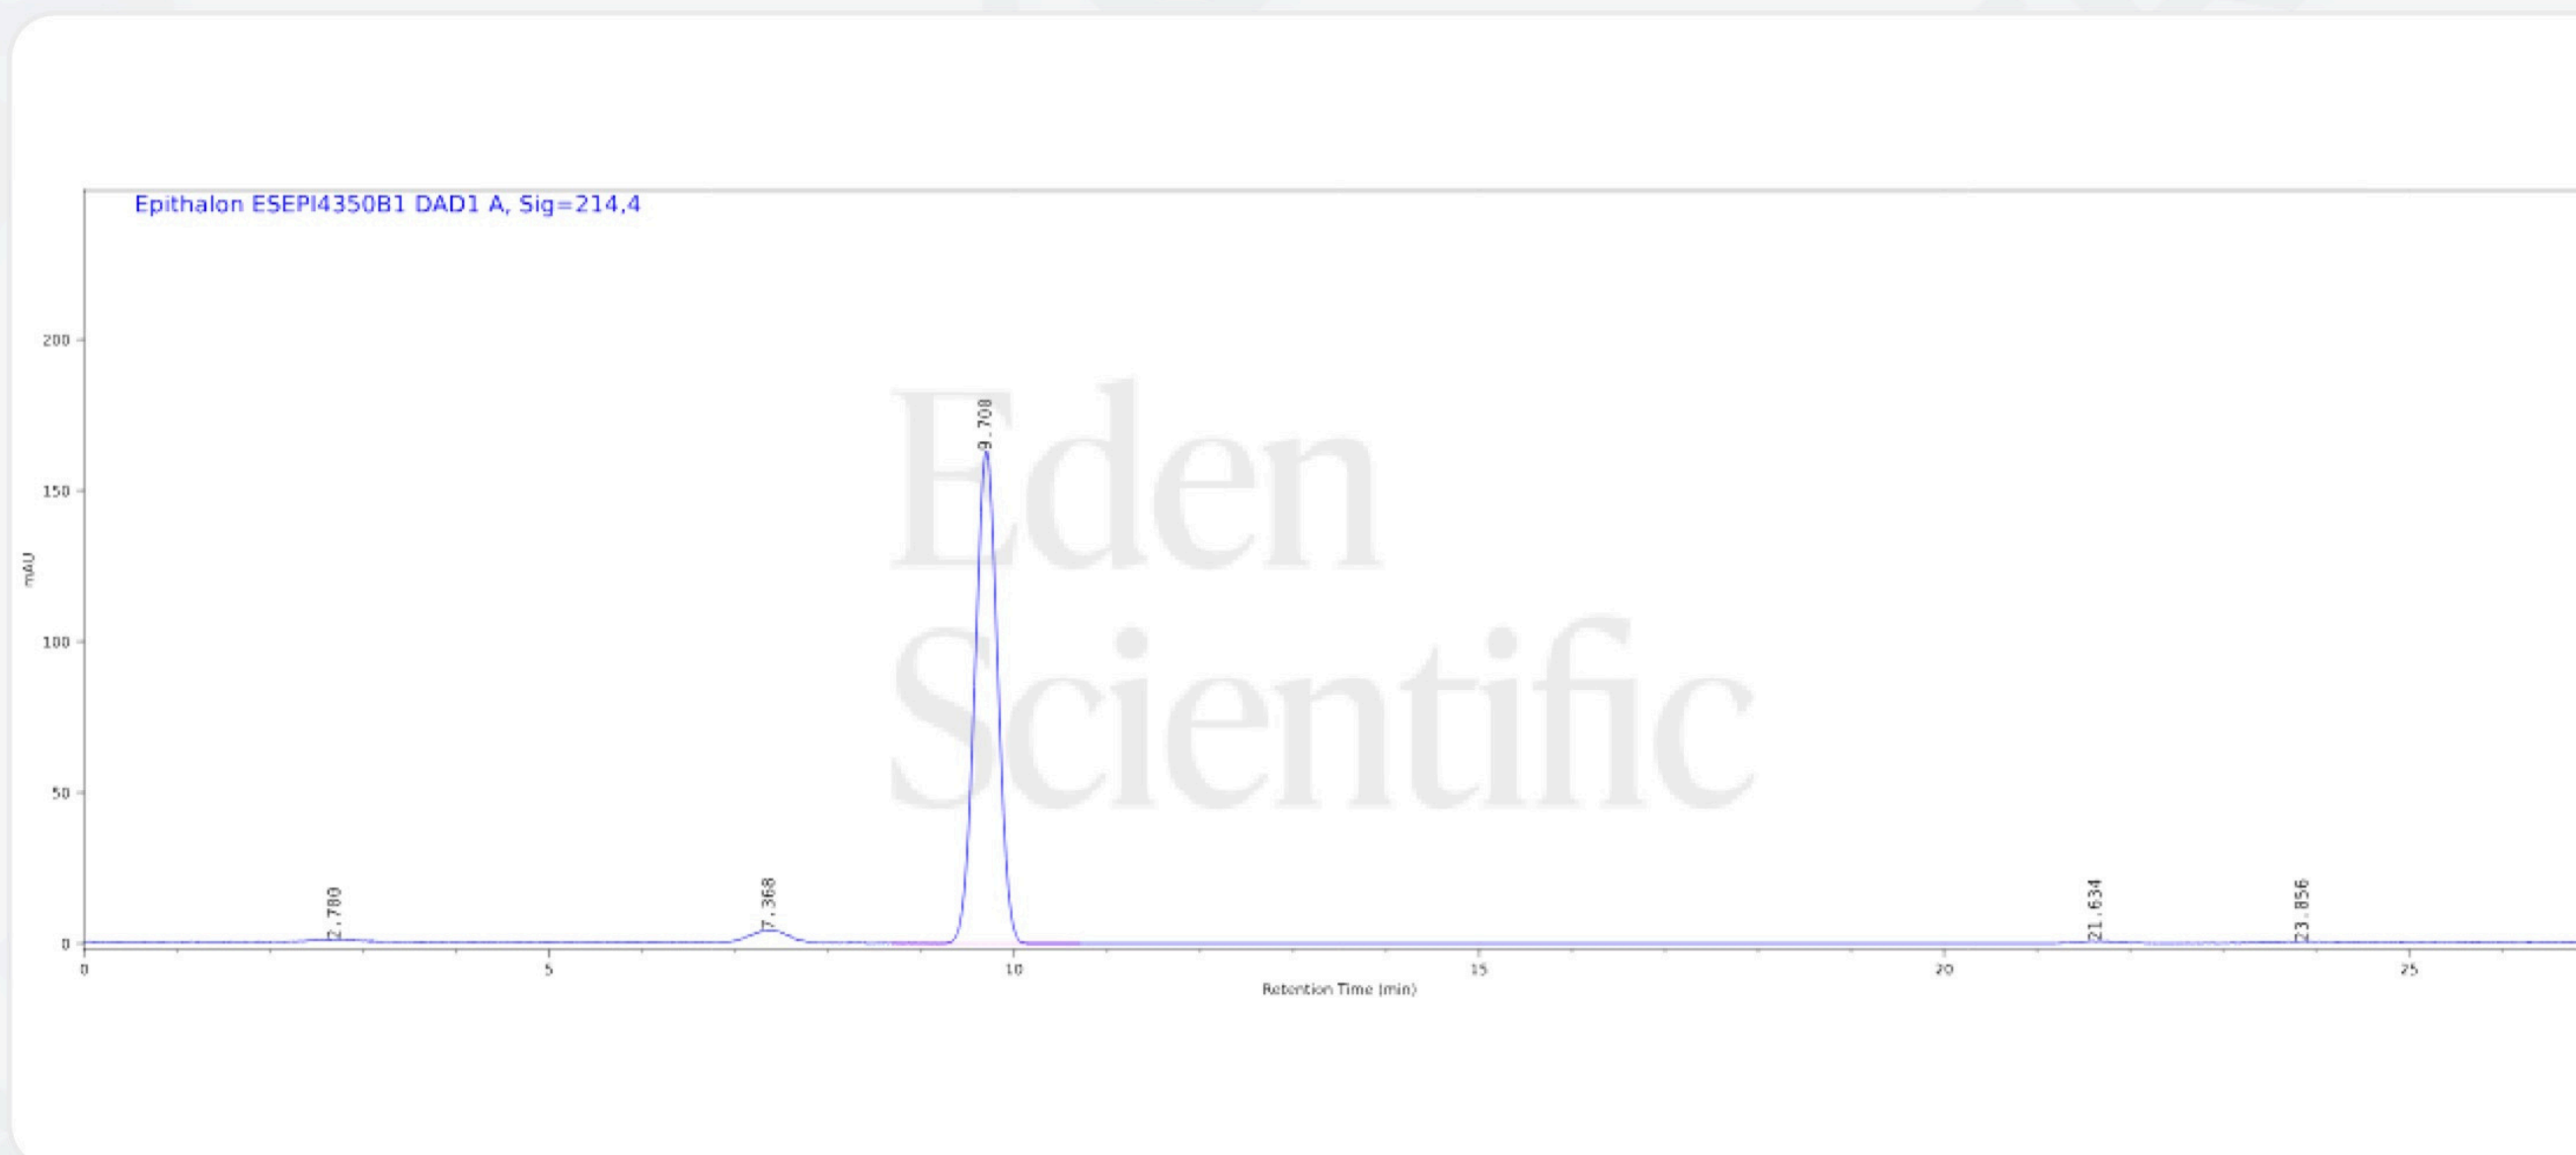

 Lab Director

koveralabs.com/verify

Report#: KVR-2026-570446

Access Code: LSACRCR

CLIENT & SAMPLE INFORMATION

CLIENT	Eden Scientific	PRODUCT NAME	Epitalon
CAS NUMBER	307297-39-8	LOT / BATCH	ESEPI4350B1
SAMPLE QUANTITY	40 mg	FORM	Lyophilized powder
TEST DATE	02/11/2026		

This Certificate of Analysis certifies that the sample listed herein was tested for microbial sterility screen in accordance with standard laboratory procedures.

TEST RESULTS

TEST	SPECIFICATION	RESULT	STATUS
Microbial Sterility Screen	No growth	No growth detected	PASS

AUTHORIZATION

PREPARED BY

Marcus Sterling, B.S.

QC Analyst

REVIEWED BY

David Cohen, M.S.

Quality Director

koveralabs.com/verify

CLIENT & SAMPLE INFORMATION

CLIENT	Eden Scientific	PRODUCT NAME	SS-31
CAS NUMBER	736992-21-5	LOT / BATCH	ES2S3450B1
SAMPLE QUANTITY	35 mg	FORM	Lyophilized powder
TEST DATE	02/11/2026		

This Certificate of Analysis certifies that the sample listed herein was tested for endotoxin safety screen in accordance with standard laboratory procedures.

TEST RESULTS

TEST	SPECIFICATION	RESULT	STATUS
Endotoxin Safety Screen	≤0.5 EU/mL	PASS	PASS

AUTHORIZATION

PREPARED BY Marcus Sterling, B.S. QC Analyst	REVIEWED BY David Cohen, M.S. Quality Director
---	---



CLIENT & SAMPLE INFORMATION

CLIENT	Eden Scientific	PRODUCT NAME	Epitalon
CAS NUMBER	307297-39-8	LOT / BATCH	ESEPI4350B1
SAMPLE QUANTITY	40 mg	FORM	Lyophilized powder
TEST DATE	02/11/2026		

This Certificate of Analysis certifies that the sample listed herein was tested for heavy metals screen in accordance with standard laboratory procedures.

HEAVY METALS SCREEN

ELEMENT	SPECIFICATION	RESULT
Lead (Pb)	< LOD	Negative
Cadmium (Cd)	< LOD	Negative
Arsenic (As)	< LOD	Negative
Mercury (Hg)	< LOD	Negative

AUTHORIZATION

PREPARED BY Liam Clarke, B.S. QC Analyst	REVIEWED BY David Cohen, M.S. Quality Director
---	---

